

The Hygrohood is an insulated humidity hood with built-in hygrometer used for non-destructive Relative Humidity testing of concrete and other floors and screeds to international standards BS8201, BS8203 and BS5325.




FEATURES



NON-DESTRUCTIVE



Place the Hygrohood in the wettest areas, as found with the Tramex CME5 & CMEX5.

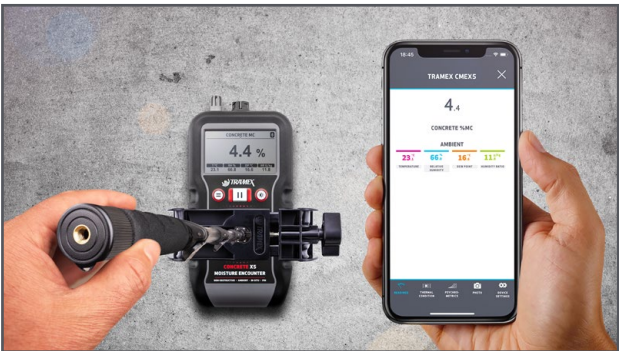

MANUFACTURERS OR NATIONAL STANDARD RECOMMENDATIONS

British Standards code of practice BS8201, BS8203, BS5325 suggests that a concrete floor or screed should be sufficiently dry to allow installation of a resilient floor covering and tested using the insulated impermeable hood method. Non-destructive moisture content tests with the Tramex CME5, CMEX5, CME4 or CMEX2 can be carried out until the floor or screed reaches the moisture level specified by the floor covering manufacturer. The Tramex CME5, CMEX5, CME4 or CMEX2 can be used to determine the areas of greatest concern on the floor or screed. At that stage relative humidity tests using the Hygrohood can be implemented to corroborate the non-destructive moisture content test.

PRE-TEST CONDITIONING AND PREPARATION

For best and most accurate results, tests should be carried out after the internal conditions of the building in which the slab is located have been at normal service temperature and humidity for at least 48 hours. All artificial heating or drying equipment should be turned off at least 96 hours before final readings are attempted, otherwise results may not accurately reflect the amount of moisture present or moisture movement in the slab during normal operating conditions. Avoid testing in locations subject to direct sunlight or sources of heat. Use of artificial aids for accelerated drying of concrete is not recommended. If they are being used it is recommended they should be turned off at least four days before taking final readings. It is advantageous to know the background of the site e.g. when the floor or screed was poured, thickness levels, etc.

TESTING

1. Before positioning the Hygrohood on the floor slab, the surface should be clear of any foreign materials and swept clean of any dust or loose materials that could affect a proper seal between the hood and the surface of the floor.
2. Using butyl tape, seal the insulated Hood to the concrete surface.
3. The Hygrometer will record minimum and maximum values while it remains switched on. Optional C°/F° units are available. Memory will be reset when the unit is switched off.

Always refer to the adhesive and/or floor covering manufacturer's recommendations for the acceptable moisture content levels of concrete floor screeds.

CALIBRATION SPECIFICATION

The Hygrometer is factory calibrated to 75%RH at 20°C. The calibration should remain stable for a minimum period one year from date of purchase unless the unit is physically damaged or misused.

The measuring range is 20% - 99%RH, with a temperature range of : 0°C - 50°C / 32° - 122°F

Tolerances : +/- 3%, +/- 1°C / +/- 2°F.

Replacement battery: CR2032.

